



Application Note

AN000540

TDC-GP30

First Hit Level Determination and Regulation over Flow and Temperature Variations

v1-00 • 2018-Sep-13

Content Guide


1	Introduction..... 3	3.1	Result of the Analysis of Amplitude 14
2	Analysis of Amplitude with Flow and Temperature Variation 8	3.2	Flow Chart 15
2.1	Measurement at Constant Flow and Constant Temperature 10	3.3	Declaration 16
2.2	Measurement at Constant Flow and Variable Temperature 11	4	Summary / Results 18
2.3	Measurement at Variable Flow and Variable Temperature 12	5	Revision Information..... 20
3	Description of Assembler Code . 14	6	Legal Information 21

1 Introduction

TDC-GP30 derives precise time-of-flight (TOF) information by evaluating the zero crossings of a received ultrasound signal. Since the received waveform has many zero crossings, a definite and unambiguous numbering of zero cross points is required for a stable and reliable measurement result. This application note gives an introduction to first hit level (FHL) regulation methods to achieve the desired stability.

As background, the TDC-GP30 transmitter generates a rectangular pulse train (“fire burst”) that gets applied to a piezo-electric transducer. After passing through the medium under test (i.e. water, gas, other fluid, etc.) the TDC-GP30 receiver detects the corresponding receive burst. Due to the transducer’s band filter characteristic, the receive burst sequence takes the shape of a sinusoidal burst signal, consisting of a sequence of waves (see Figure 1) When properly configured the TDC-GP30 can precisely determine the arrival time of a specific wave’s zero crossing point that will be used for Time-of-Flight (TOF) measurements. The selected zero crossing points are converted into digital edge signals which define the received hits.

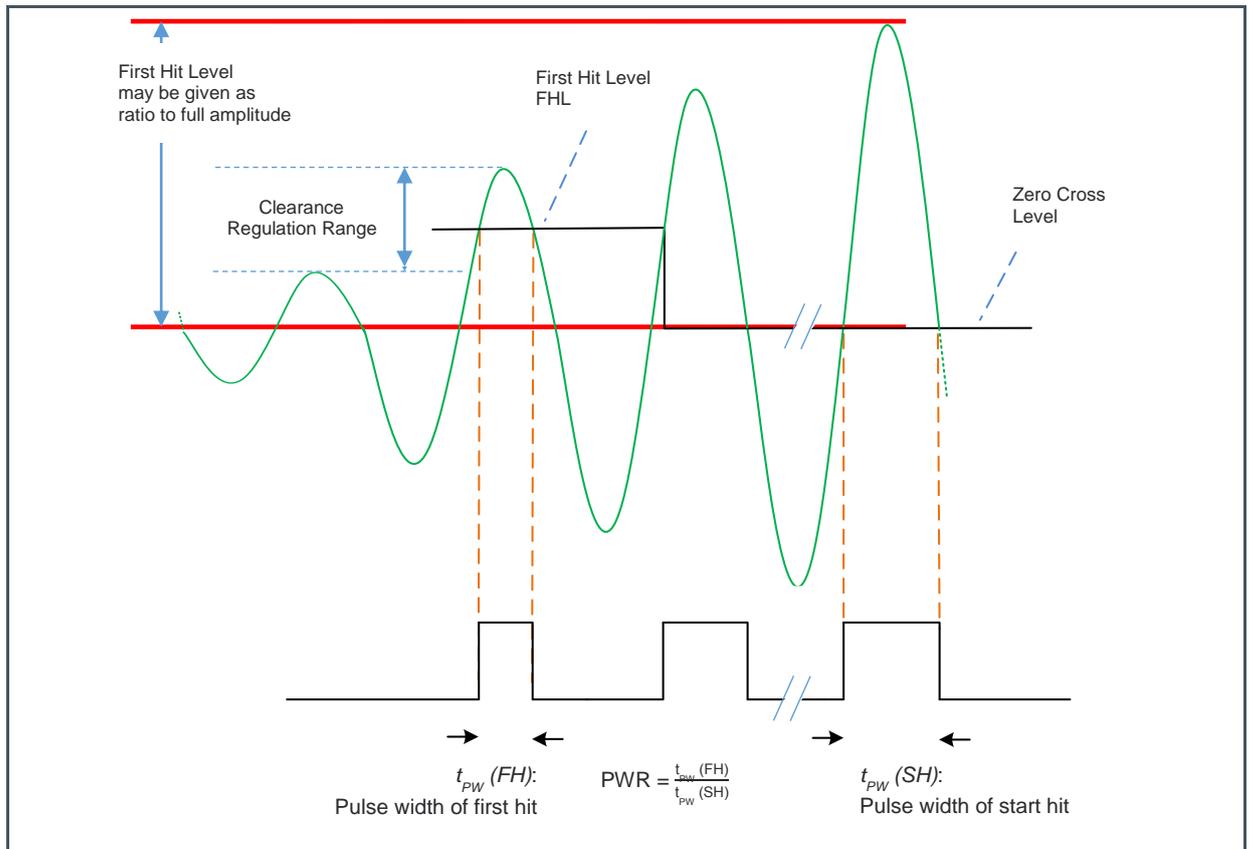Figure 1:
First Wave Detection



For the TOF measurement, typically a sequence of received hits is used. This sequence begins at the so-called “start hit” (SH). The length of this sequence as well as the position of the start hit are defined by the user. For example, the SH could be defined as the 8th received hit after the so-called “first hit” (FH). This way, the first hit is utilized to consistently determine the relative position of the receive hit sequence within the receive burst. This application note discusses how to consistently determine a stable FH position.

TDC-GP30 offers an amplitude and pulse width measurement of the receive wave to define and determine a stable FH. Below are the steps to accomplish this:

- 1. ANALYZE WAVES:** Measure the first few received signal wave amplitudes individually, using the TDC-GP30. (see section 2 “Analysis of Amplitude with Flow and Temperature Variation”). Figure 1 shows four received waves with increasing peak amplitude.
Note: It is possible to monitor the receive burst waveform signal using an oscilloscope. Please use caution as impedance loading from the scope probe will likely influence the measured signal.
- 2. DETERMINE FIRST HIT (FH):** Compare the peak amplitude of each wave to the amplitude of its immediate predecessor wave. The wave with the highest amplitude difference from the preceding wave is a good candidate to be chosen for defining the first hit (FH). In Figure 1 the second visible wave is determined to define the first hit (FH).
- 3. DEFINE CLEARANCE REGULATION RANGE AND FIRST HIT LEVEL (FHL):** The amplitude range between the peak of the first hit’ wave and the peak of its immediate predecessor is called the “clearance” regulation range. The first hit level FHL, different from the zero cross level, will be used going forward to determine the first hit FH. The FHL is a threshold amplitude level chosen to be between the peak values of the FH wave and the preceding adjacent wave. Figure 1 shows the clearance range between the first and second waves with the FHL defined within that range.
- 4. START HIT (SH):** The “start hit” (SH) is chosen as a fixed subsequent hit, for example the eighth hit after the FH. Note that it is not recommended to use the first hit itself or its direct successor as SH, since these two hits are not referenced to the zero cross level, but rather to the FHL (see Figure 1). Other selection criteria for the definition of SH, like increased noise of early hits or possible interference, are beyond the scope of this application note.
- 5. PULSE WIDTH RATIO (PWR):** The first hit’s pulse width $t_{pw}(FH)$ is measured at the wave which defines the first hit as the time interval between when the instantaneous receive amplitude rises above the FHL, crests and then decreases to below the FHL. It is shown in red dashed lines on the left side in Figure 1. The pulse width $t_{pw}(SH)$ of the SH is shown in red dashed lines on the right side in Figure 1. Note that $t_{pw}(SH)$ refers to the time interval between the zero crossings of the corresponding wave. The “pulse width ratio” (PWR) is the ratio of $t_{pw}(FH) / t_{pw}(SH)$. PWR has some maximal value when FHL is close to the preceding wave’s peak level and approaches 0 when the FHL approaches the next wave’s peak amplitude. PWR is thus a figure of merit than can be used in subsequent TOF measurements to help keep the FHL clear from levels where the first hit detection might erroneously switch to an undesired neighboring wave.

This procedure is the first important step of the FHL selection. Until here, determining FHL is not related to firmware functionality and can be used in remote control operation as well. But now it should be noted that the result of the selection process described above can change over temperature, production tolerances and aging. For some devices and transducers it may even depend on flow and pressure. The goal is to obtain reliable and stable first hit detection under the influence of all these different factors. Upcoming sections of this document discuss determining the first hit (FH) under different environmental conditions.



Information

The definition of the FHL can be thought of in several different contexts as follow:

- FHL as configurable value (System Handling Registers, addresses 0x0DA / 0x0DB)
Parameters ZCD_FHL_U / ZCD_FHL_D are from -255 to 255
- FHL as physical value (voltage of FHL_U / FHL_D), 1 LSB = 0.88 mV
Voltages V_{FHL_U} / V_{FHL_D} are from -224 mV to 224 mV

The actual physical value is $V_{FHL} = \pm 0.88\text{mV} * \text{ZCD_FHL}$


The Pulse Width Ratio can also be used to track FHL.



Information

Sometimes it may make sense to choose a FHL using narrower clearance range. This may improve stability over temperature variations.

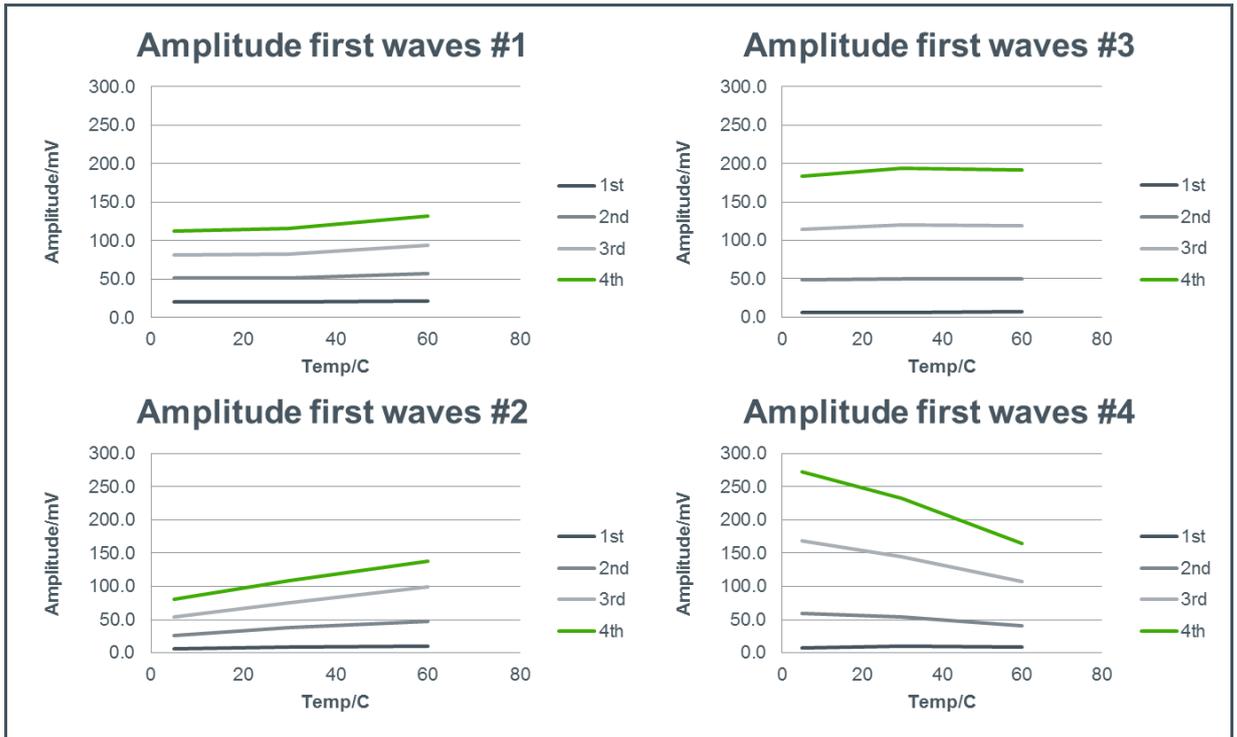
Figure 2:
Different Trends of Amplitude



These example plots demonstrate how different receive wave amplitudes - and with them the corresponding FHL levels – can vary over temperature for different spool pieces #1 - #4. Accordingly, different spool pieces may require different FHL regulation methods for stable first hit detection.

In the next section a spool piece with following behavior is used.

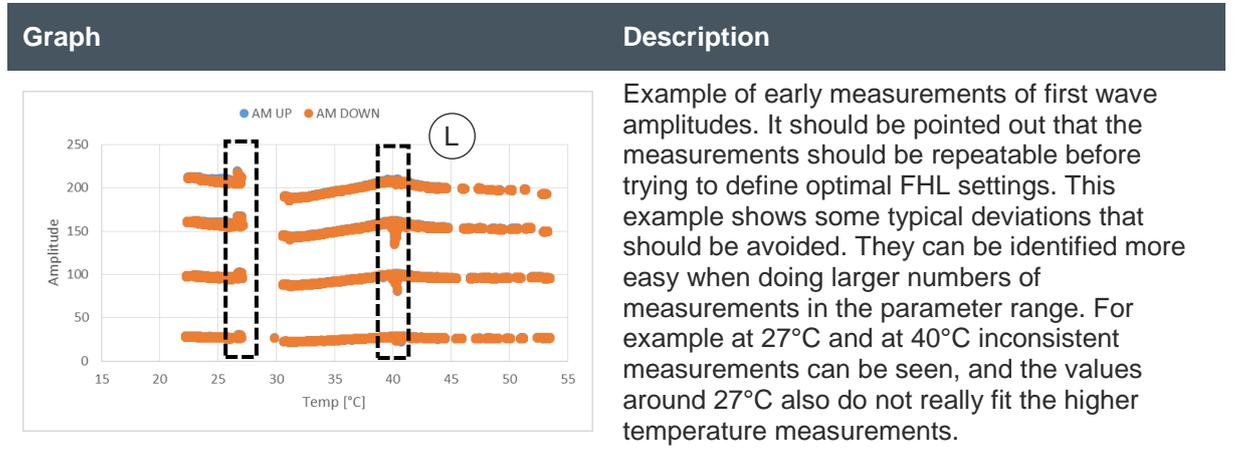Figure 3:
Amplitude First Waves



2 Analysis of Amplitude with Flow and Temperature Variation

First, it is necessary to examine the variation of amplitudes of the individual waves of the receive burst within the operating range (temperature and flow).

The next subsections will illustrate different situations. As introduction, FHL, PWR and amplitude are shown at constant flow and temperature. Next, the influence of temperature variation is shown. And finally the temperature and flow variations cover the full operating range.

From these data the limits for PWR and FHL can be extracted.

Now follows an abstract description of what to do to accomplish this analysis.

GP30 Configuration:

Start with a well working configuration at zero flow and change only the following points.

- Post Processing disable
- Watchdog disable
- Every calibration (e.g. ZC, AM, HSCLK) after each measurement
- AM Measurement stops after 1st Hit
- (PWR Measurement needs at least 3 Hits)

Process of data collection:

- Configure GP30
- Start with defined flow and temperature and with FHL = min
- Start loop to measure amplitude (AM) until FHL = max
 - Measure amplitude with GP30
 - Increase FHL (e.g. by step)
- After each pass of the loop, vary the flow and start the loop again.
- As soon as the flow range had been covered, vary the temperature and start the loop over the flow range again.
- Analyze the data collection to define limits for FHL and therefore PW

Parameter Range:

- First Hit Level
 - FHL max = 200
 - FHL min > = 5
 - FHL step = 2
- Numbers of collected Values (e.g. 2 or more)
- Pump Control
- Averaged (e.g. 4)

Collected Values:

- | | |
|------------------|--|
| • FHL UP/DOWN | First hit level measured by GP30 |
| • TOF1 UP/DOWN | First TOF value measured by GP30 |
| • PWR UP/DOWN | Pulse width ratio measured by GP30 |
| • AM UP/DOWN | Received amplitude measured by GP30 |
| • DIFF TOF | Calculated by GP30 Evaluation software |
| • SUM TOF | Calculated addition of measured SUMTOF AVG UP/DOWN |
| • Temp [°C] | Water temperature, measured with external sensor |
| • Flow [l/h] | Flow rate, measured with external sensor |
| • Flow Avg [l/h] | Averaged flow rate, measured with external sensor |

**Information**




Due to the difficulty of keeping the temperature constant with different flow rates, it is advisable to collect the data in a good pace.

To get a first and quick overview of the analysis, only low and high temperature would be helpful.

2.1 Measurement at Constant Flow and Constant Temperature

- Flow = zero flow
- Temperature = ~19 °C

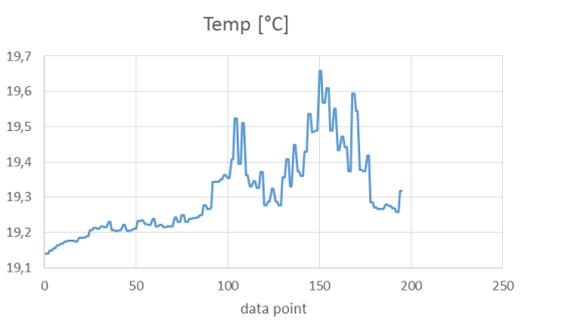
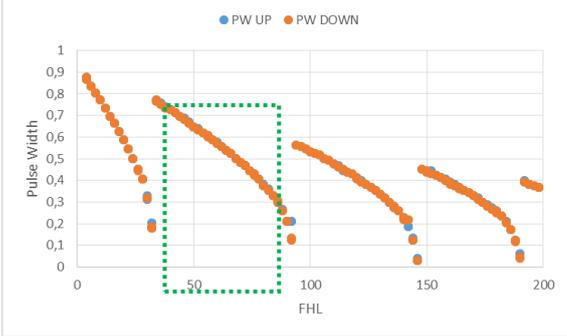
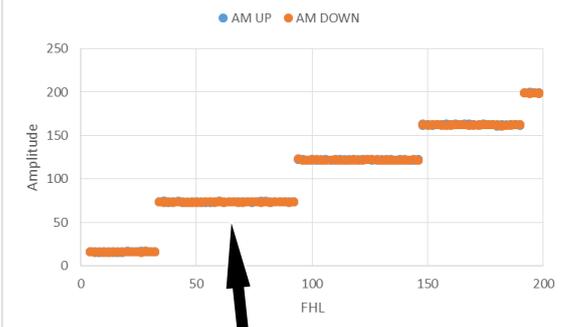
Figure 4:
Measurement at Constant Flow and Constant Temperature

Graph	Description
	<p>Measured water temperature. It is not important to keep the temperature very constant. It only has to cover the required area.</p>
	<p>Pulse width vs. FHL. The pulse width approaches zero with increasing FHL, and jumps to a high value again when jumping to the next wave (compare next graph). The green area marks a good range for the FHL level to stay with the same wave over chosen temperature.</p>
	<p>Measured amplitude of the first wave vs. FHL. With increasing FHL, the first hit detection jumps to the next wave when FHL exceeds the peak amplitude. At these steps, the amplitude of the next wave is measured and PWR jumps to a high value (see above). At the same point, the measured TOF also changes (not shown). The graph shows amplitudes of first 5 waves of receive burst, measured by increasing the FHL (zero flow, fixed temperature). The difference between neighboring amplitudes is the clearance, indicated by the width of the lines. The bigger the clearance the better FHL mode will work.</p>

2.2 Measurement at Constant Flow and Variable Temperature

- Flow = zero flow
- Temperature = 20 °C to 55 °C

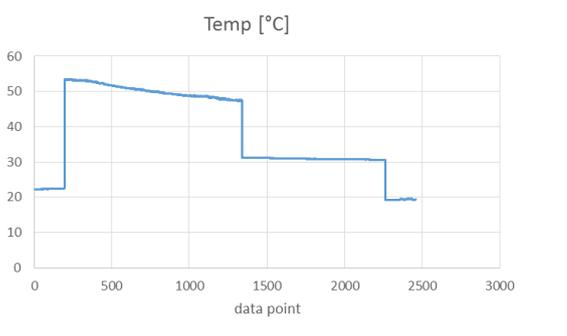
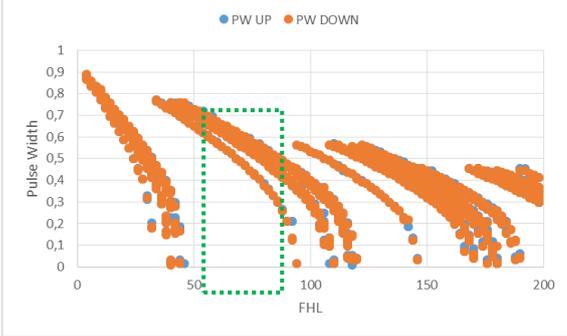
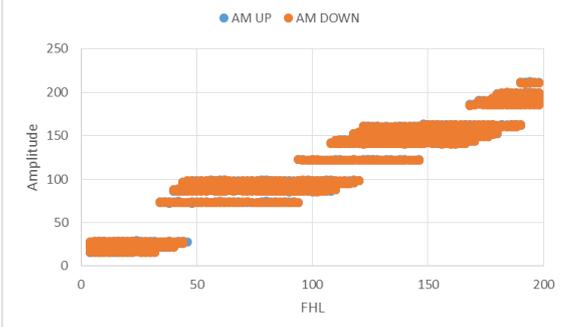
Figure 5:
Measurement at Constant Flow and Variable Temperature

Graph	Description
	<p>Again, it is not necessary to set a dedicated temperature but to vary it.</p> <p>The water temperatures of the test points should cover the desired operation range.</p>
	<p>The pulse width gets smaller with increasing FHL, and gets high again when jumping to the next wave. Also the temperature has an impact and broadens the spread of PWR for a given wave.</p> <p>The green area marks a good range for the FHL level to maintain the same first wave over the whole temperature range. Due to temperature variation this is narrower than for a fixed temperature.</p>
	<p>Amplitudes of first 5 waves of receive burst, measured by increasing the FHL (zero flow, fixed temperature).</p> <p>Shows the difference between them = clearance. The bigger the clearance the better FHL mode will work.</p>

2.3 Measurement at Variable Flow and Variable Temperature

- Flow = 0 l/h – 850 l/h
- Temperature = low (20 °C) and high (50 °C)

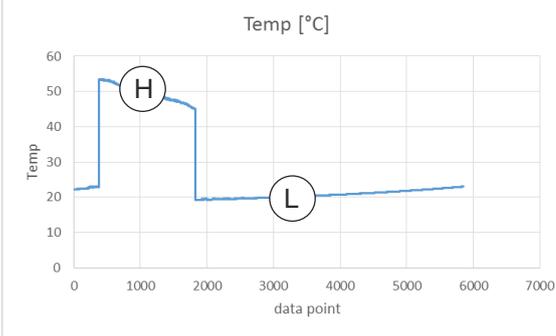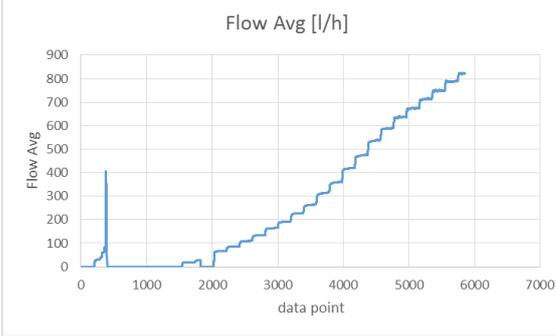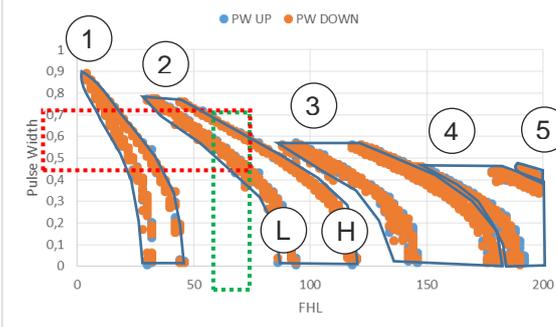Figure 6:
Measurement at Variable Flow and Variable Temperature

Graph	Description
	<p>Again, it is not necessary to set a dedicated temperature but to vary it.</p> <p>It only has to cover the required area.</p> <p>“H” and “L” marked the high and low temperature.</p>
	<p>It is not necessary to set a dedicated flow but to vary it and to measure it. The flow variation shall cover the full operating range.</p>
	<p>The pulse width gets smaller with increasing FHL, and gets high again when jumping to the next wave. Also the temperature and flow have an impact and broaden the spread of PWR for a given wave.</p> <p>The green area marks a good range for the FHL to stay with the same wave over the whole operating range. Due to temperature and flow variation this further narrowed.</p> <p>55 < FHL < 70 (means between 48.4 mV and 61.6 mV)</p> <p>Accordingly the PWR varies from 0.43 to 0.71 (red area)</p> <p>The blue frame stands for the first to the fifth wave. “H” and “L” marked the pulse width at high and low temperature.</p>

Graph	Description
	<p>Amplitudes of first 5 waves of receive burst, measured by increasing the FHL (zero flow, fixed temperature). Shows the difference between them = clearance. The bigger the clearance the better FHL mode will work.</p> <p>The blue frame stands for the first to fifth wave. "H" and "L" marked the amplitude at high and low temperature.</p>

3 Description of Assembler Code

3.1 Result of the Analysis of Amplitude

The following values were obtained due to the spool piece shown in section 2.3 Measurement at Variable Flow and Variable Temperature.

3.1.1 Coarse FHL Regulation to Stay in the Range

Only when leaving the range, the firmware will increase or decrease the FHL to be in the range again. For increased FHL regulation lower deviation of regulation "clearance".

The range for regulation "clearance": $55 < \text{FHL} < 70$
accordingly the PWR varies from 0.43 to 0.71

After configuration of GP30 with initial FHL (for this spool piece, $\text{FHL} = 62$) and setup following parameter:

PWR_LIMIT_MAX (7fpp) = 0x5A (= decimal 90 --> 0.703125)
PWR_LIMIT_MIN (7fpp) = 0x37 (= decimal 55 --> 0.4296875)

3.1.2 Permanent FHL Regulation

Compared to our flow firmware, the regulation will be done permanently and also indicates when you are outside the configured range.


New range for regulation "clearance": $\text{FHL} = 62$
accordingly the new PWR varies from 0.54 to 0.65

For a permanent FHL regulation set min and max to the same value.

PWR_LIMIT_MAX (7fpp) = 0x4C (= decimal 76 --> 0.59375)
PWR_LIMIT_MIN (7fpp) = 0x4C (= decimal 76 --> 0.59375)

3.2 Flow Chart

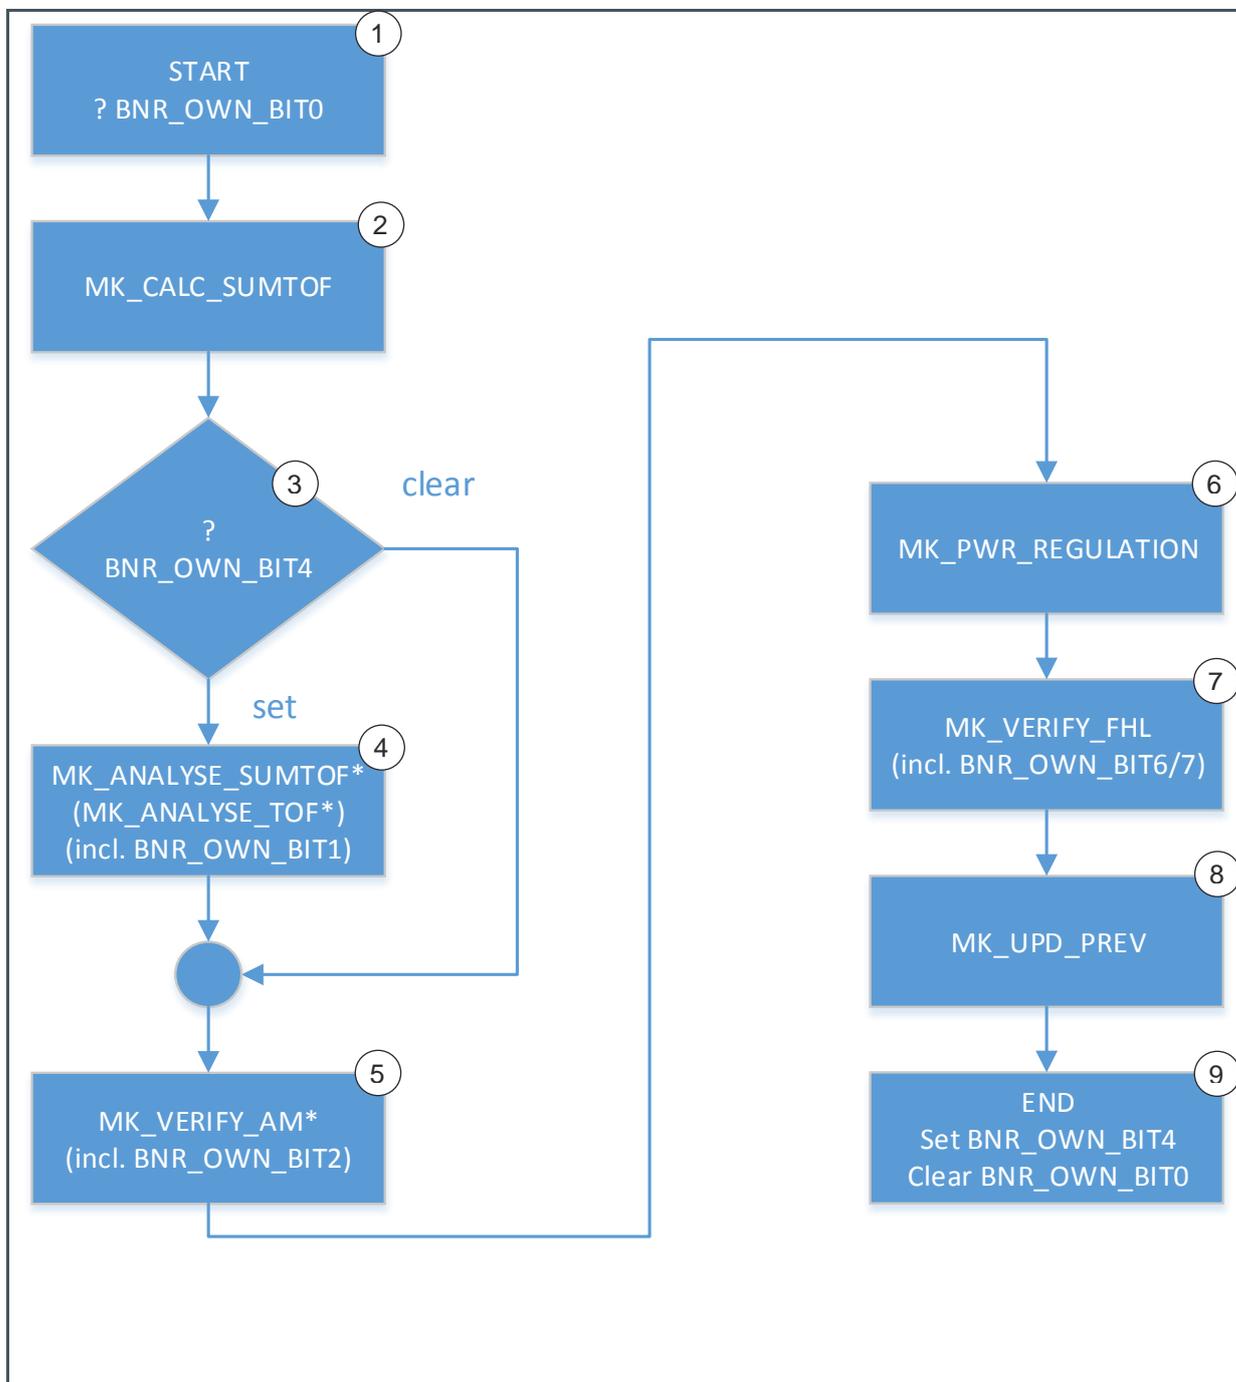Figure 7 :
Flow Chart



- 1 START
As long as BNR_OWN_BIT0 is set, the FHL calculation is executed
- 2 MK_CALC_SUMTOF
Calculates the SUMTOF
- 3 BNR_OWN_BIT4
Will be set at the end of FHL calculation
- 4 MK_ANALYSE_SUMTOF* (MK_ANALYSE_TOF*)
Remark: This block is not completely integrated in the FHL Regulation.
Analysis of the SUMTOF (TOF UP / TOF DOWN) will be executed after the second run if there is a period jump, BNR_OWN_BIT1 is set and stops further FHL calculation
- 5 MK_VERIFY_AM*
Remark: This block is not completely integrated in the FHL Regulation.
Compares current AM (UP and DOWN) with AM_LIMIT_MIN otherwise BNR_OWN_BIT2 is set or cleared
- 6 MK_PWR_REGULATION
regulates the first hit level (UP and DOWN) depends on the pulse width ratio
- 7 MK_VERIFY_FHL
verifies previous FHL with current FHL (UP and DOWN) and depends on any difference BNR_OWN_BIT6/7 is set or cleared.
- 8 MK_UPD_PREV
store current values as previous parameters to verify with next values
- 9 END
At the end, set BNR_OWN_BIT4 and clear BNR_OWN_BIT0 to indicate that the FHL calculation is done



Information

Further details about each subroutine are shown in the assembler source code.

3.3 Declaration

Figure 8:
Declaration

CONST	Value	Description
OWN_FLAG	0x50	Own Flag Register
BNR_OWN_BIT0	0	Bit Number, FHL Calculation (jump into subroutine and clear at the end)
BNR_OWN_BIT1	1	Bit Number, ERROR: period jump, cleared not implemented (t.b.d.)
BNR_OWN_BIT2	2	Bit Number, ERROR: amplitude under minimum limit, cleared by subroutine
BNR_OWN_BIT4	4	Bit Number, "1" = FHL Calculation (first run was completed)
BNR_OWN_BIT5	5	Bit Number, "1" = Zero Cross Calibration was done

CONST	Value	Description
BNR_OWN_BIT6	6	Bit Number, "1" = FHL_UP Regulation is active
BNR_OWN_BIT7	7	Bit Number, "1" = FHL_DOWN Regulation is active
AM_LIMIT_MIN	0x41	Compare to FDB_US_AM_U and FDB_US_AM_D (e.g. 0x2E000)
PWR_LIMIT_MAX	0x42	7fpp (0.7 = decimal 90 = 0x5A) initialized in subroutine MK_FWI_FHL1
PWR_LIMIT_MIN	0x43	7fpp (0.3 = decimal 38 = 0x27) initialized in subroutine MK_FWI_FHL1
FDB_US_SUMTOF_ADD_ALL	0x44	Calculated SUMTOF
FDB_US_SUMTOF_ADD_ALL_PREV	0x45	Previous calculated SUMTOF
FDB_US_TOF_0_U_PREV	0x46	Previous TOF0_UP value
FDB_US_TOF_0_D_PREV	0x47	Previous TOF0_DOWN value
SHR_ZCD_FHL_U_PREV	0x48	Previous FHL_UP value
SHR_ZCD_FHL_D_PREV	0x49	Previous FHL_DOWN value
SUMTOF_LIMIT	0x40000	SUMTOF_LIMIT multiplied by 250ns/2 ¹⁶ = 1us
HALF_T_REF	0x20000	1/2 * T reference = 1/2 * 0x40000 * 250ns/2 ¹⁶ = 1/2 * 1us
FW_ROMVERSION_REV	0xA1	ROM Class + ROM Version
FW_VERSION_NUM	0xF20000	Special FW ("F" = FW Class + FW Version) (0x00 to 0xFF)
FW_VERSION_MAJ	0x000000	FW Major Revision (0x0 to 0xF)
FW_VERSION_MIN	0x000000	FW Minor Revision (0x0 to 0xF)
FW_VERSION_BLD	0x000000	Build Number (0x00 to 0xFF)
FW_VERSION	FW_VERSION_NUM + FW_VERSION_MAJ + FW_VERSION_MIN + FW_VERSION_BLD	



Attention

Following CONST parameter are not completely integrated in the simple FHL Regulation

- AM_LIMIT
- SUMTOF_LIMIT
- HALF_T_REF

4 Summary / Results

Depending on the requirements of the ultrasonic flow meter, spool piece and transducers, the first hit level needs to be regulated or simply it can be used a fixed first hit level over temperature and over flow.

For a stable and dependable FHL regulation process, irregular events have to be considered. These events are not taken into account in the preceding example:

- Empty spool piece - how can the regulation resume to the desired state without knowledge of the prior state (e.g. medium temperature).
The same applies to correct initialization.
- Aging of the sensor (transducers, aging of the spool piece by deposits,...) and /or changing amplitude of the received signal for any other reason.
- Change of required FHL by flow Measurement at different temperatures
e.g. heat meter is running with cold water and hot water.
- Limited criteria of FHL
e.g. what is the minimum and maximum FHL.
- Corrupted measurement (bubbles etc.) should always be excluded from FHL regulation.
Criteria for detection of corrupted measurements have to be developed and implemented.
- It should be noted that in this ASM source code the FHL regulation for UP and DOWN is independent of one another.

Alternatively TDC-GP30-F01, including the flow firmware offers a number of auxiliary measurements and settings to support stable first hit detection:

- Peak amplitude measurement of selected waves of the receive signal
- First hit pulse width ratio (PWR) measurement to optimize the quality of the first hit detection
- Automated zero crossing calibration
- First hit level setting to detect the chosen wave at some particular amplitude

The available regulation methods in overview:

- Method 1, Keep FHL constant
- Method 2, Return to a trusted FHL in case of inconsistency
- Method 3, Offset trusted FHL
- Method 4, Fallback method

Any of these methods can be combined with the following options:

- Option A, Regulate PWR
- Option B, Define FHL as ratio to receive amplitude
- Option C, Activate FHL regulation modes only in failure case



For further information about flow firmware, please refer to the following document:

- TDC-GP30-F01 datasheet volume 4 “Firmware, Memory and ROM Overview”
Get in touch with your nearest channel partner or sales office
-

5 Revision Information

Changes from previous version to current revision v1-00	Page
Initial version for release	

- Page and figure numbers for the previous version may differ from page and figure numbers in the current revision.
- Correction of typographical errors is not explicitly mentioned.

6 Legal Information

Copyrights & Disclaimer

Copyright ams AG, Tobelbader Strasse 30, 8141 Premstaetten, Austria-Europe. Trademarks Registered. All rights reserved. The material herein may not be reproduced, adapted, merged, translated, stored, or used without the prior written consent of the copyright owner.

Information in this document is believed to be accurate and reliable. However, ams AG does not give any representations or warranties, expressed or implied, as to the accuracy or completeness of such information and shall have no liability for the consequences of use of such information.

Applications that are described herein are for illustrative purposes only. ams AG makes no representation or warranty that such applications will be appropriate for the specified use without further testing or modification. ams AG takes no responsibility for the design, operation and testing of the applications and end-products as well as assistance with the applications or end-product designs when using ams AG products. ams AG is not liable for the suitability and fit of ams AG products in applications and end-products planned.

ams AG shall not be liable to recipient or any third party for any damages, including but not limited to personal injury, property damage, loss of profits, loss of use, interruption of business or indirect, special, incidental or consequential damages, of any kind, in connection with or arising out of the furnishing, performance or use of the technical data or applications described herein. No obligation or liability to recipient or any third party shall arise or flow out of ams AG rendering of technical or other services.

ams AG reserves the right to change information in this document at any time and without notice.

RoHS Compliant & ams Green Statement

RoHS Compliant: The term RoHS compliant means that ams AG products fully comply with current RoHS directives. Our semiconductor products do not contain any chemicals for all 6 substance categories, including the requirement that lead not exceed 0.1% by weight in homogeneous materials. Where designed to be soldered at high temperatures, RoHS compliant products are suitable for use in specified lead-free processes.

ams Green (RoHS compliant and no Sb/Br): ams Green defines that in addition to RoHS compliance, our products are free of Bromine (Br) and Antimony (Sb) based flame retardants (Br or Sb do not exceed 0.1% by weight in homogeneous material).

Important Information: The information provided in this statement represents ams AG knowledge and belief as of the date that it is provided. ams AG bases its knowledge and belief on information provided by third parties, and makes no representation or warranty as to the accuracy of such information. Efforts are underway to better integrate information from third parties. ams AG has taken and continues to take reasonable steps to provide representative and accurate information but may not have conducted destructive testing or chemical analysis on incoming materials and chemicals. ams AG and ams AG suppliers consider certain information to be proprietary, and thus CAS numbers and other limited information may not be available for release.

Headquarters

ams AG
Tobelbader Strasse 30
8141 Premstaetten
Austria, Europe
Tel: +43 (0) 3136 500 0

Please visit our website at www.ams.com

Buy our products or get free samples online at www.ams.com/Products

Technical Support is available at www.ams.com/Technical-Support

Provide feedback about this document at www.ams.com/Document-Feedback

For sales offices, distributors and representatives go to www.ams.com/Contact

For further information and requests, e-mail us at ams_sales@ams.com